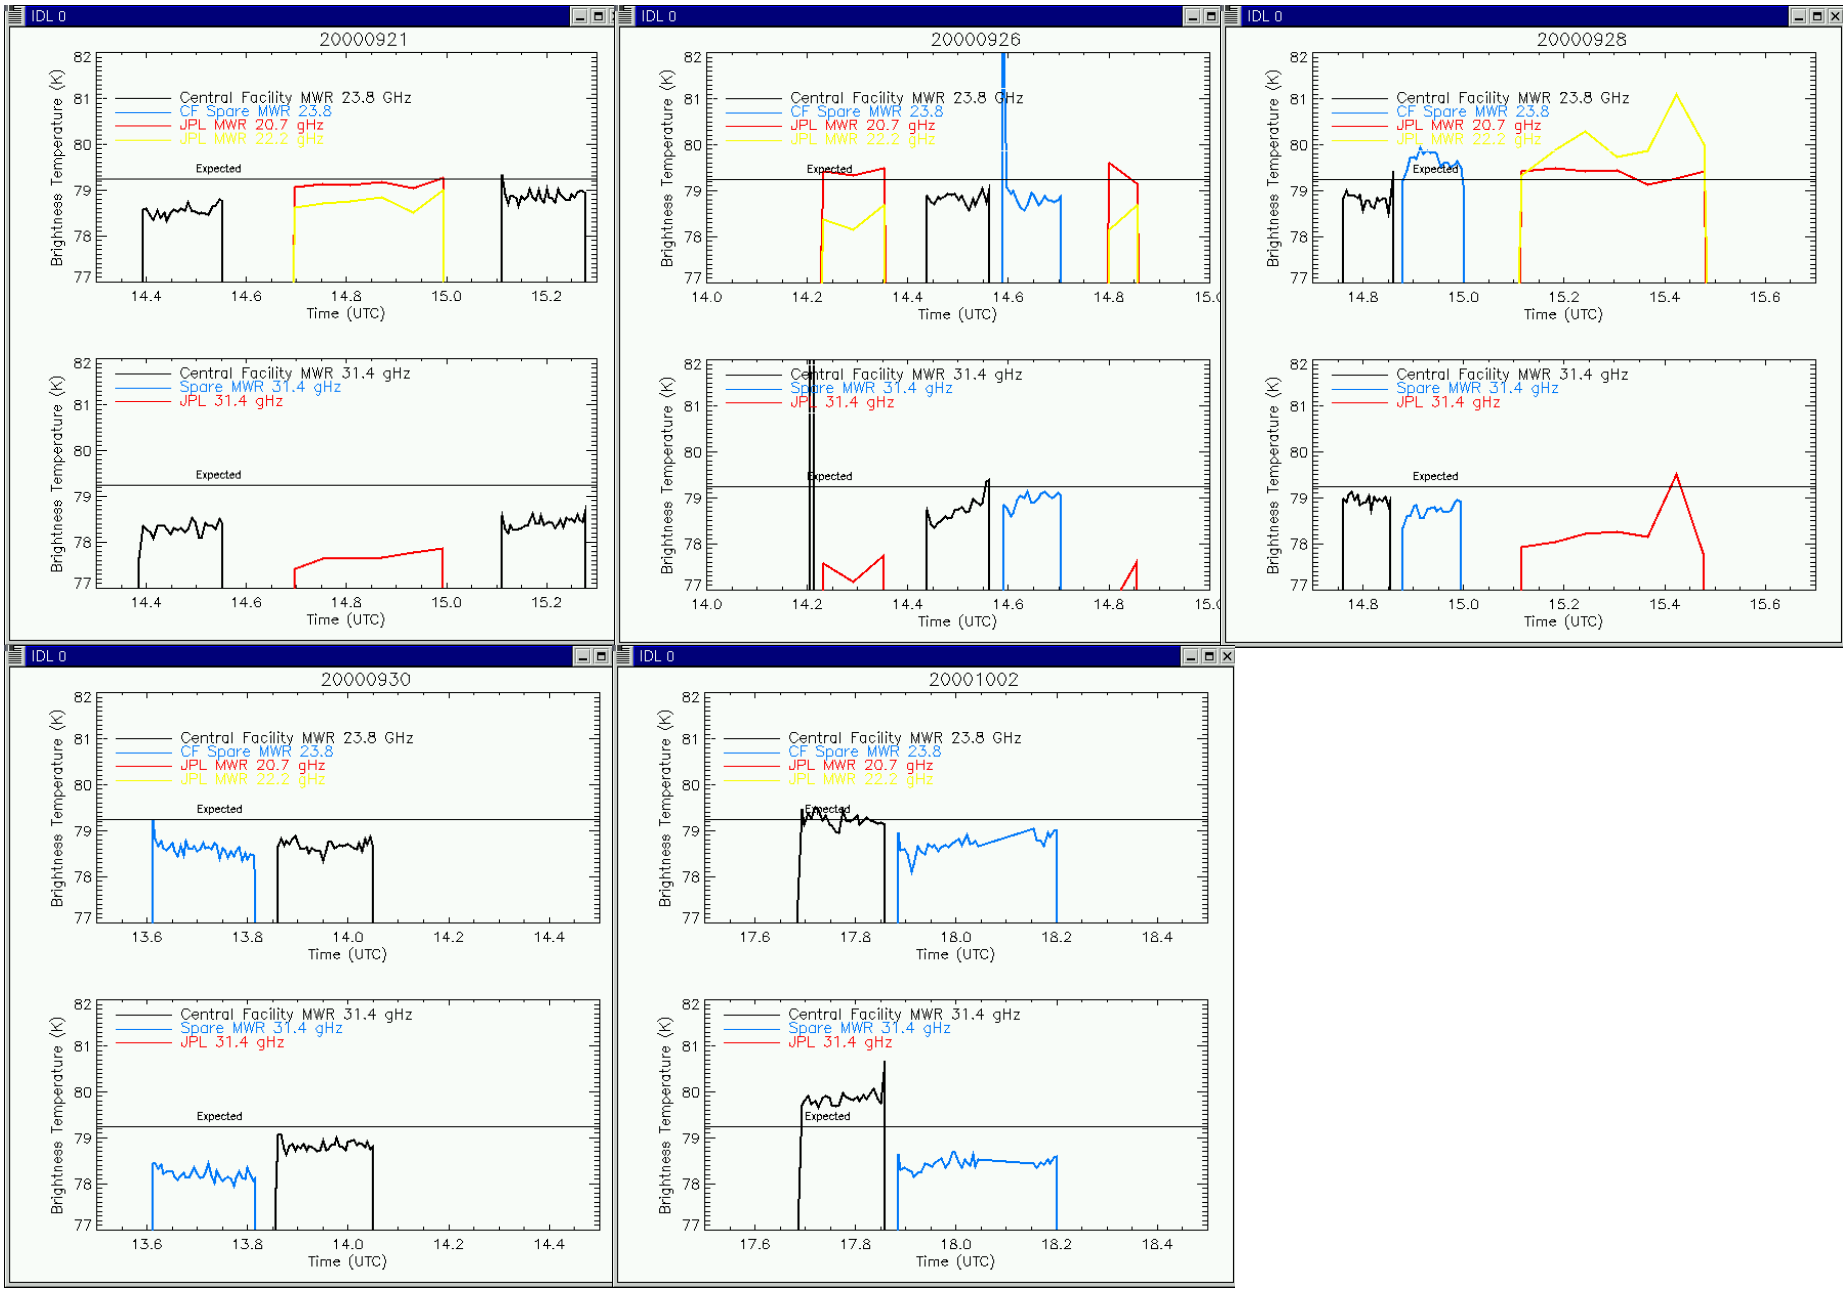
IDL 0
20000921
Central Facility MWR 23.8 GHz
CF Spare MWR 23.8
JPL MWR 20.7 gHz
JPL MWR 22.2 gHz
Expected
Brightness Temperature (K)
Time (UTC)
Central Facility MWR 31.4 gHz
Spare MWR 31.4 gHz
JPL 31.4 gHz
IDL 0
20000926
IDL 0
20000928
IDL 0
20000930
IDL 0
20001002